


Experimental Setup of USM1400-LT TERS

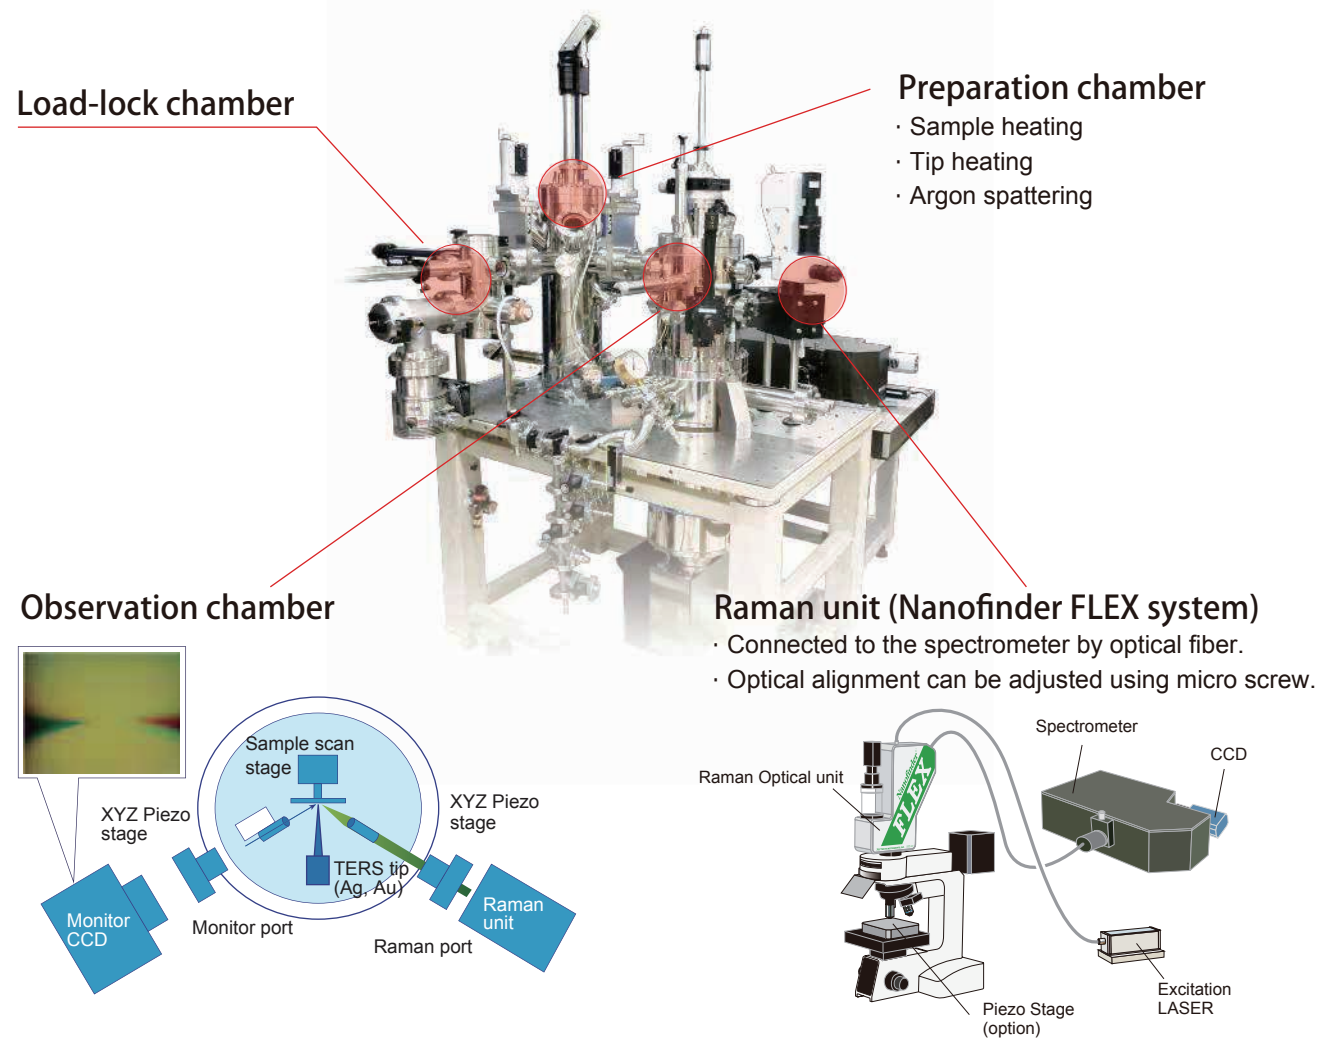

Specifications

■ Observation Chamber

Temperature : 5.5 K-Room temperature
Vacuum Base : 3.0×10^{-8} Pa

■ STM head

Scan Range : $1 \times 1 \times 0.25 \mu\text{m}$ @5.5 K
STM spatial resolution : Atomic resolution

■ Raman spectroscopic system

Incident angle : 35°
Lens : Aspheric lens (NA 0.35)

■ Raman spectroscopic system

Spectrometer : $f=35$ cm or 50 cm, $F\text{-number}=3.8$
Spectral resolution : 2 cm^{-1} @550nm, 1200 G/mm

■ Laser for excitation

- Standard:
 - Fiber output (FC connector:2 m)
 - Output variable (ND filter)
- Excitation wavelength:
 - Nd : Yag laser (532 nm, 25 mW)
 - Option : He-Ne Laser (633 nm)


USM1400-LT TERS

(Based on USM1400 Scanning Probe Microscope-LT TERS)

Low Temperature (LT)-UHV/Tip Enhanced Raman Spectroscopy

World' s first single molecule imaging method by low temperature (LT).

Under LT UHV condition, it can realize sub-nanometer scale Raman spectroscopic imaging with improved S/N ratio and sensitivity.

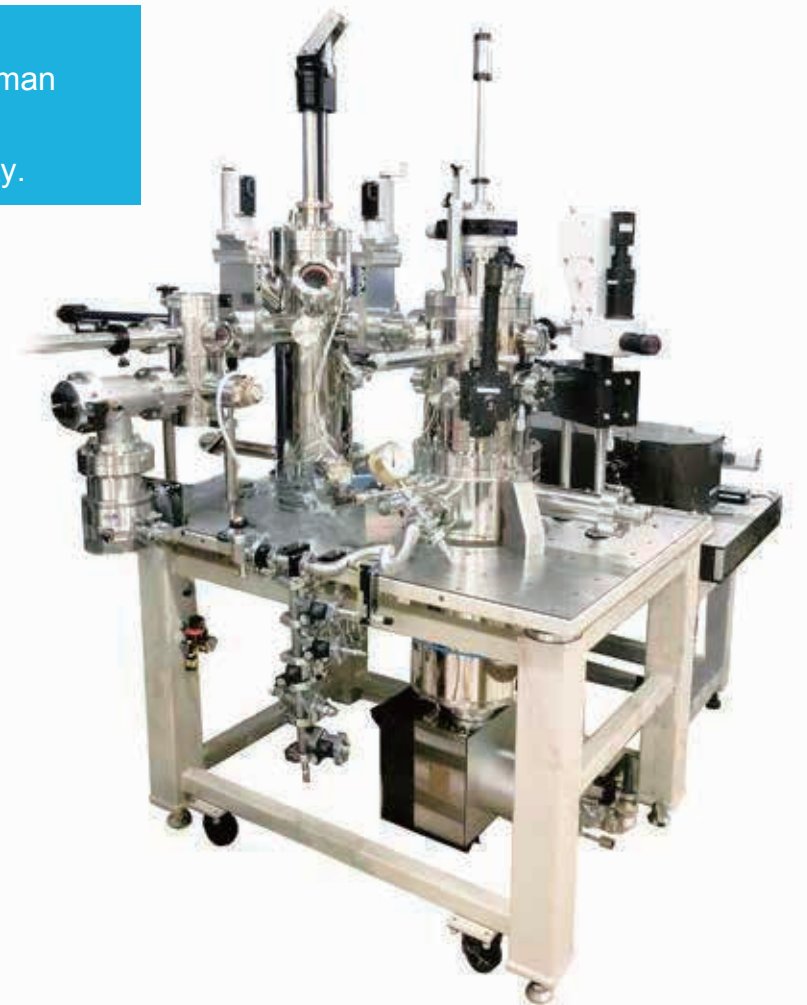

Application

- Molecule' s bonding state of single molecular.
- Topography observation & elements identification.
- Lattice defect' s identification.
- UHV deposition layers' Raman and topographic evaluation.

UNISOKU Co., Ltd. 

E-mail: info@unisoku.co.jp Web site: <http://www.unisoku.co.jp/>


2-4-3 Kasugano, Hirakata, Osaka 573-0131 Japan TEL +81-72(858)6456 FAX +81-72(859)5655

20180622

UNISOKU
TII Group

About Tip-Enhanced Raman Spectroscopy (TERS)

TERS is the ultimate combination of two well proven techniques. It combines the strength of Raman Spectroscopy and Scanning Probe Microscopy. The optical intensity is enhanced by the near field effect around the conducting STM tip – with the result of a strong localisation of the optical signal. Single molecule spectra become detectable within minutes.

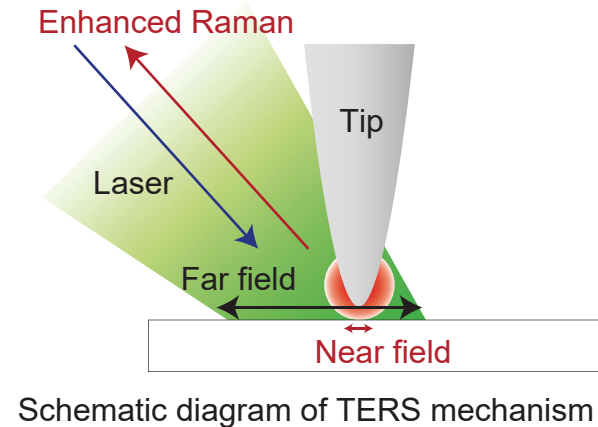

USM1400 - LT TERS (Based on USM1400 Scanning Probe Microscope-LT TERS)

Optical access with high collection efficiency is realized by mounting a lens with 3D adjustment by a piezo motor on the SPM stage under low temperature, high vacuum. Combined with confocal Raman spectroscopic system, high stability tip enhanced Raman scattering imaging (TERS) is achievable. It is a new device that can image the bonding state of molecules and crystals in sub-nanometer scale.

Features


- The USM1400 SPM system as the base provides proven STM and AFM imaging capability in UHV LT
- *in-situ* optical elements provide optimal focusing and high intensity for the optical signals
- The seamless interface to TII' s renowned Nanofinder FLEX™ provides an efficient and easy to use turnkey solution
- The spatial resolution for Raman image is nanometer scale (<10nm)
- High enhancement factor of TERS by using Ag tip.
- Sample temperature from RT down to 5K and the UHV environment guarantee ultimate stability of the measurements at high intensity – and avoid degradation of sensitive organic samples
- *in-situ* deposition on cold and clean substrates is available by the modular expandability by adding organic and inorganic deposition sources.

Application example

Chemical image and topographic image

Example : TERS mapping results of Carbon nanotube

G-band and D-band TERS mapping of CNT on silver substrate were observed. Defect of Carbon nanotubes are observed as energy filtered image in comparison with a topographic image.

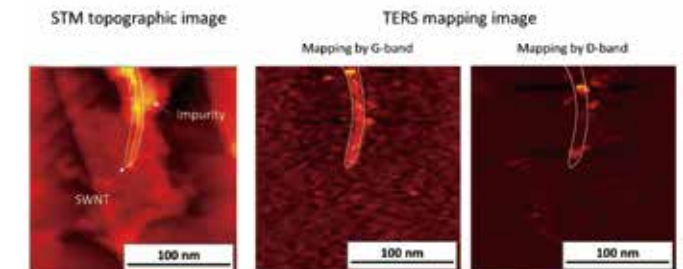


Stable measurements of TERS signal using low temperature (LT) condition.

Time resolved measurements of TERS spectra of 1,2-Di(4-pyridyl) ethylene(DPE) at RT and LT (Liq-N₂) condition.

A sequence of TERS spectra is measured at the same location. TERS spectra observed at low temperature (Liq N₂) conditions are more stable than that of RT.

Low temperature prevents the degradation of the sample

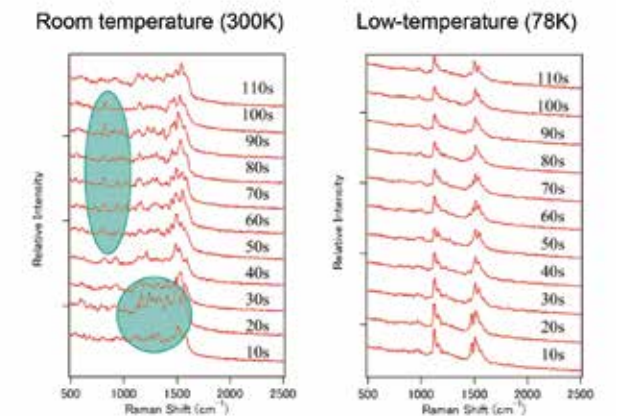

High spatial resolution reached "Single molecular level "

Co-deposited ZnTPP and H₂TPP form an alternating chain of molecules on an Ag substrate. Subsequently Local Raman spectra have been taken in the indicated spots. (blue = H₂TPP; red = ZnTPP adsorption sites). The related spectra reveal distinct differences which can be attributed to the differing chemical bonding states of H₂TPP as exposed to ZnTPP.

Single molecular resolution in Raman spectroscopy

Zinc tetraphenylporphyrin (ZnTPP) + meso-tetraphenylporphyrin (H₂TPP) on Ag measurements and DFT calculation by S. Jiang + Z. Dong + et. al. *Nature nanotechnology* 10, 865-869 (2015)

